

## 1. Report summary

### 1.1. Test Laboratory

Contact	Philip DePalo
E-mail address	drphil@consultology.us

### 1.2. Tested Organization

Name	InnoVision Medical
Mailing address	19 South Street 21202 Baltimore MD United States

### 1.3. Tested System(s)

IHE N.A. Connectathon 2021		
Product Name	Version	Owner
Medical Gateway	1.0.5	Eldon Metz
This testing session was held from 3/1/21 to 3/5/21		

### 1.4. Report identification

This report has been generated on 3/5/21 with identifier 2021.NA.Connectathon.IMT.20210305142112

### 1.5. Disclaimer

This report summarizes the outcome of the testing performed by InnoVision Medical during the event : IHE N.A. Connectathon 2021. It includes information about success and failure and should only be used internally. This report does not certify the capabilities of any commercial product offered by InnoVision Medical. Potential purchasers of the organization's products should consult any IHE Integration Statements [<http://product-registry.ihe.net>] published by the organization to confirm the IHE profiles and actors supported by its products.

## 2. System : Medical Gateway (1.0.5)

### 2.1. Results per Integration Profile/Actor/Option

Results per Integration Profile/Actor/Option				
Integration Profile	Actor	Option	Type	Result
Device Enterprise Communication	Device Observation Reporter	None	T	Pass
Device Enterprise Communication	Device Observation Reporter	Waveform Content Module	T	Pass
Medical Equipment Management Device Management Communication	Device Management Information Reporter	None	T	Did not complete
Consistent Time	Time Client	None	T	Pass

T: thorough / S: supportive

### 2.2. Test instances summary

Test instances summary				
Tests	Performed	Passed	Failed	Partially verified
6	8	6	0	2

Tests: the number of individual test cases run during the session

Performed: the total number of test instances performed (This count does not take into account the aborted, still running and not verified test instances)

Passed/Failed: the number of test instances verified and set to passed/failed by a monitor

Partially verified: the number of different test instances that was reviewed but on which some work still need to be done

### 2.3. Test instance details (per Integration profile/Actor/Option)

In the next sub-sections, performed test instances are gathered by Integration profile / Actor / Option. For each of the test instances, the detailed informations are available by following the link.

#### 2.3.1. Device Enterprise Communication / Device Observation Reporter / NONE

See below the details of the test instances performed for this Integration Profile/Actor/Option

Test (Meta Test)	#	Opt	Verified	Failed	Partially V
<a href="#">DEC_DOR_DOC_One_to_One_Comm</a>	3	R	<a href="#">71764</a> (kirwan) <a href="#">71776</a> (crouzier) <a href="#">72079</a> (crouzier)		
<a href="#">DEC_Multiple_DORs_DOCs</a>	1	R	<a href="#">72263</a> (paulsherman)		
<a href="#">DEC_Multiple_DORs_DOFs_DOCs</a>	1	R			
<a href="#">DEC_Standalone_DOF_w_DOR_and_DOC</a>	1	O			
<a href="#">DEC_With_ADT_Demographics</a>	1	O			
<a href="#">DEC_With_ADT_Unsuccessful</a>	1	O			

### 2.3.2. Device Enterprise Communication / Device Observation Reporter / WCM

See below the details of the test instances performed for this Integration Profile/Actor/Option

Test (Meta Test)	#	Opt	Verified	Failed	Partially V
<a href="#">DEC_w_WCM_Option_Basic</a>	3	O	72251 (kirwan)		

### 2.3.3. Medical Equipment Management Device Management Communication / Device Management Information Reporter / NONE

See below the details of the test instances performed for this Integration Profile/Actor/Option

Test (Meta Test)	#	Opt	Verified	Failed	Partially V
<a href="#">MEMDMC_DMIR_DMIC_DMIC_Unavailabl</a>	1	R			72556 (monroe)
<a href="#">MEMDMC_DMIR_DMIC_One_to_One</a>	1	R			72555 (monroe)
<a href="#">MEMDMC_Multiple_DMIRs_Multiple_D</a>	1	R			

### 2.3.4. Consistent Time / Time Client / NONE

See below the details of the test instances performed for this Integration Profile/Actor/Option


Test (Meta Test)	#	Opt	Verified	Failed	Partially V
<a href="#">CT_Client_Synch</a>	1	R	71760 (sineiheisel)		

## 2.4. Statistics

This section gathers some statistics on test instances. Only passed, failed and partially verified test instances are represented there.

### 2.4.1. Test instances per domain


Below is the distribution of test instances performed according to the various IHE domains your system was registered for.

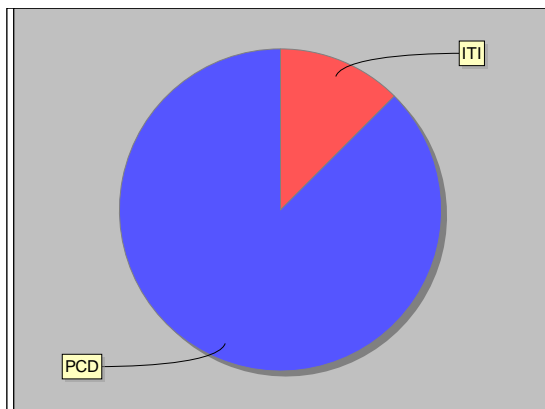

Domain	nb of TI
ITI	1
PCD	7

### 2.4.2. Test instances per integration profile


Below is the distribution of test instances performed according to the various IHE integration profiles your system was registered for.

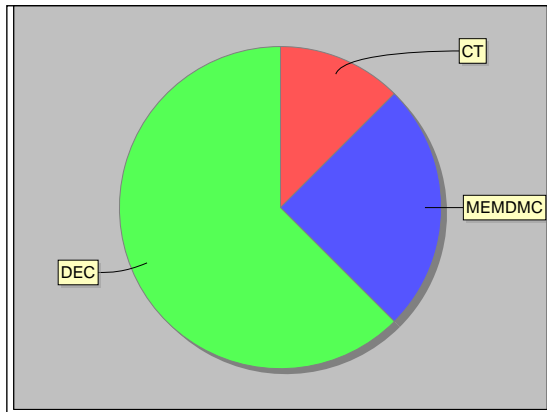

Integration profile	nb of TI
CT	1
DEC	5
MEMDMC	2

### 2.4.3. Test instances per actor


Below is the distribution of test instances performed according to the various IHE actors your system was registered for.

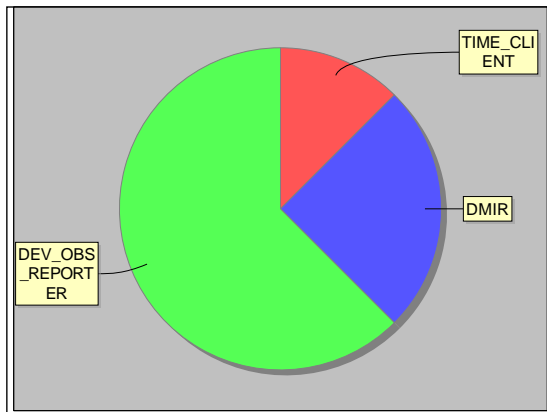

Actor	nb of TI
TIME_CLIENT	1
DEV_OBS_REPORTER	5
DMIR	2

### 2.4.4. Test instances per partner (organization level)


Below is the distribution of test instances performed per peer organization

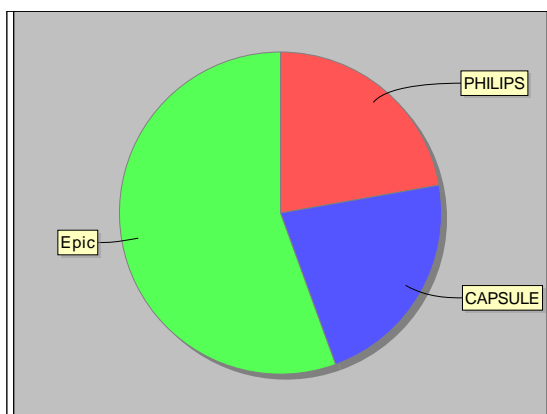

Organization	nb of TI
PHILIPS	2
Epic	5
CAPSULE	2

### 2.4.5. Test instances per partner (system level)


Below is the distribution of test instances performed per peer system

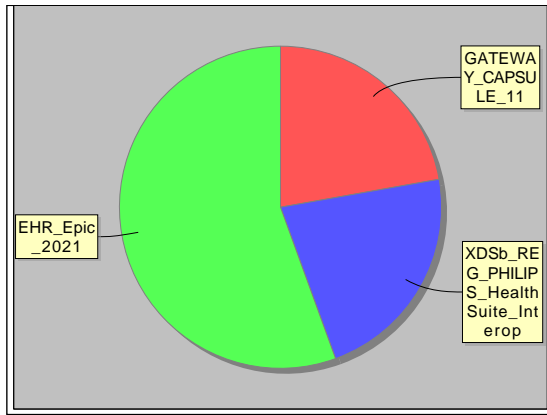

System	nb of TI
EHR_Epic_2021	5
GATEWAY_CAPSULE_11	2
XDSb_REG_PHILIPS_HealthSuite_Interop	2

### 2.4.6. Test instances per monitor

Below is the distribution of test instances verified per monitor

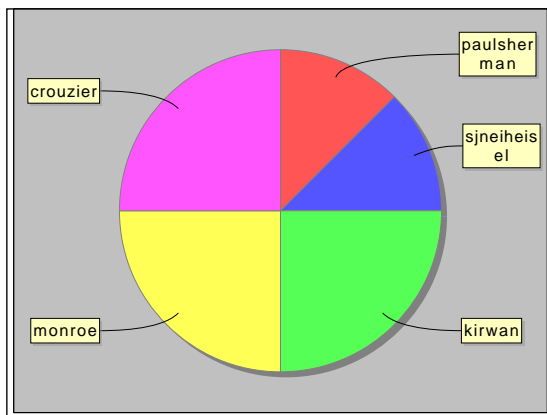

Monitor	nb of TI
kirwan	2
monroe	2
crouzier	2
paulsherman	1
sineiheisel	1

The line below indicates the end of this report, any text below this line is not part of the initial content of this report